




# ENDOSCOPE CHANNEL GUIDE




## EVIS™ 40/140/240 & EXERA™ 160-Series GI Endoscopes

**WARNING:** This guide is only a summary of the connections used for reprocessing EVIS™ AND EXERA™ endoscopes. Be sure to follow the detailed steps outlined in the *ENDOSCOPE REPROCESSING MANUAL* that was included with your endoscope when purchased.

### CONNECTION OF CHANNEL PLUG & INJECTION TUBE

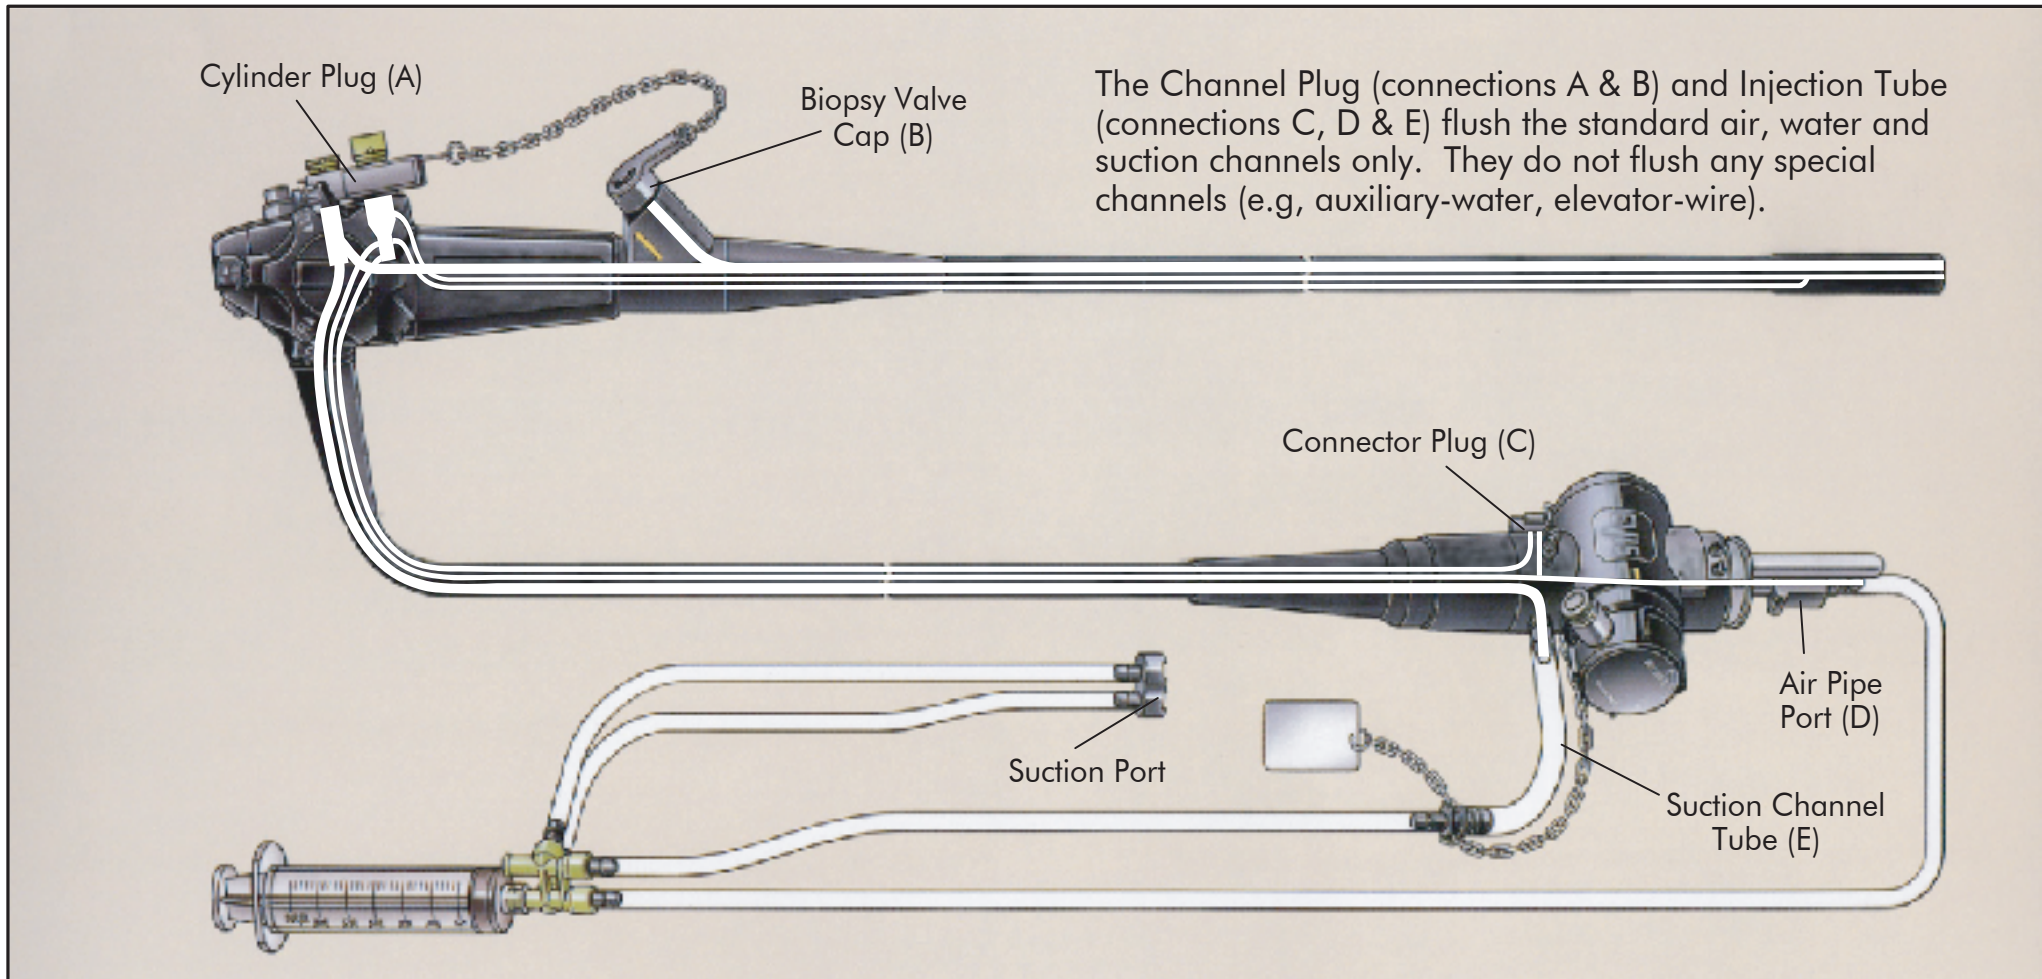


### SPECIAL CHANNELS - AUXILIARY WATER & ELEVATOR WIRE

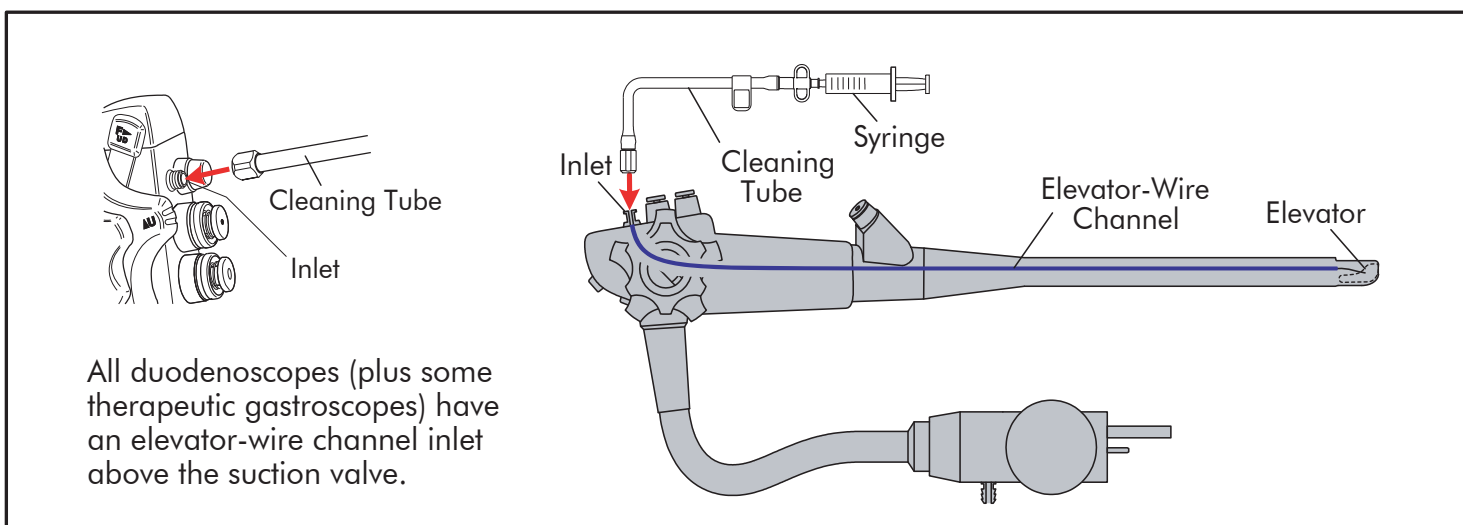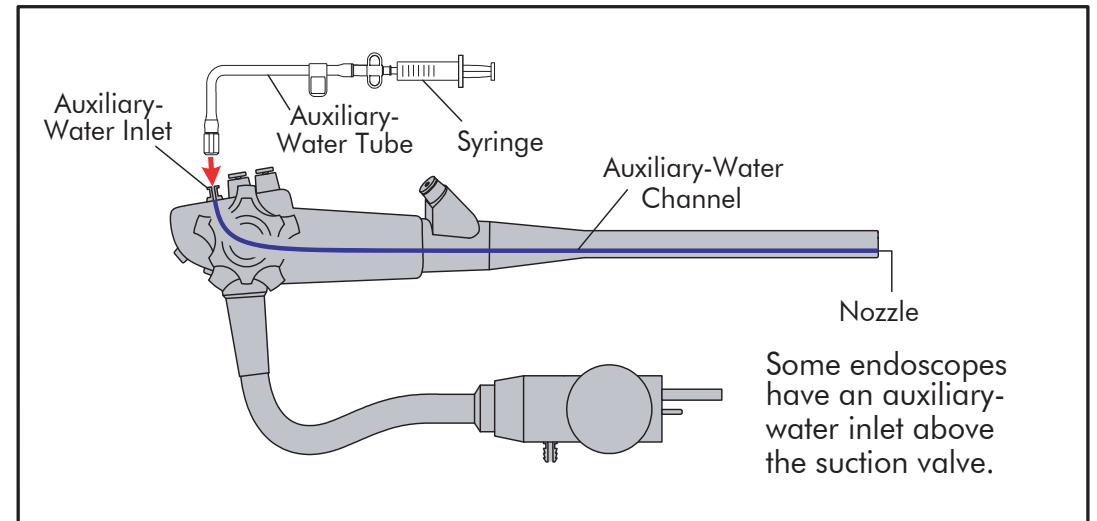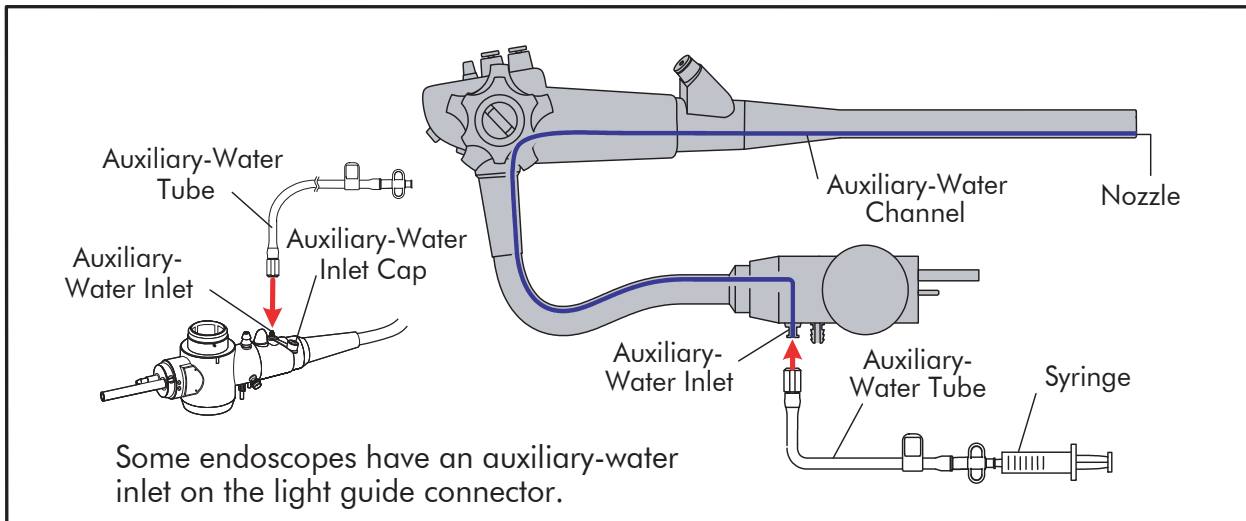

### IMPORTANT

- Failure to properly clean and high-level disinfect endoscopic equipment after each examination can compromise patient safety.
- Every channel of the endoscope must be reprocessed each time the endoscope is used, even if the channel was not utilized during the preceding patient procedure.
- Certain endoscopes have two biopsy/suction channels. Refer to the endoscope's instruction manual for information specific to these models.
- Every channel must go through every reprocessing step (cleaning, disinfection, rinsing, alcohol-air drying).
- If an automated reprocessor is used, make sure that all channels are being properly reprocessed. Follow all manufacturers' instructions.

### STANDARD CHANNELS - AIR, WATER & SUCTION

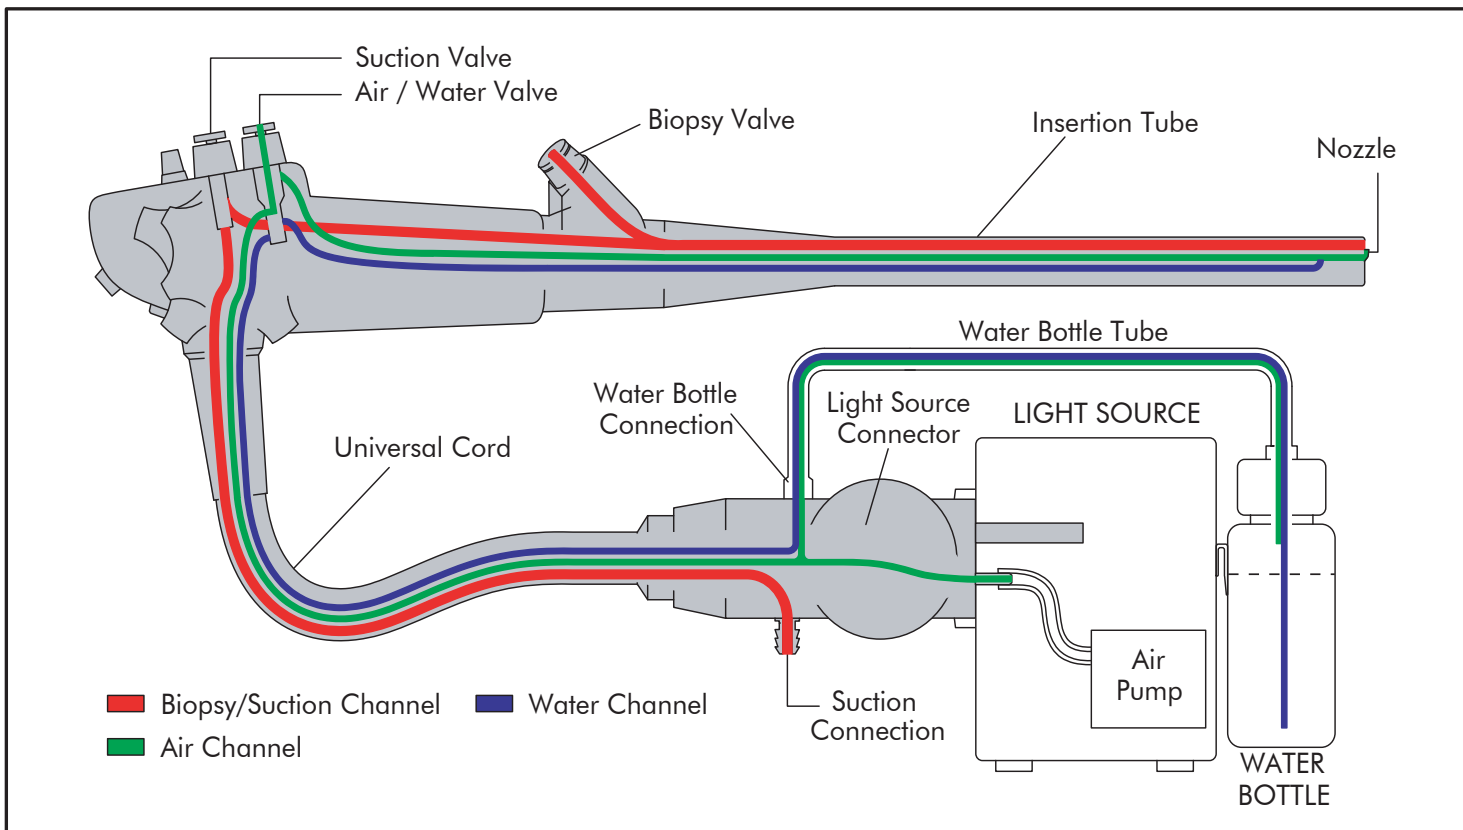

**OLYMPUS CUSTOMER SERVICE CENTER**  
800-848-9024

IF YOU HAVE ANY QUESTIONS,  
CONTACT YOUR LOCAL  
OLYMPUS REPRESENTATIVE

